

# Comparison of StimulOX™, ORC®, and MgO<sub>2</sub> Jar Test Dissolved Oxygen

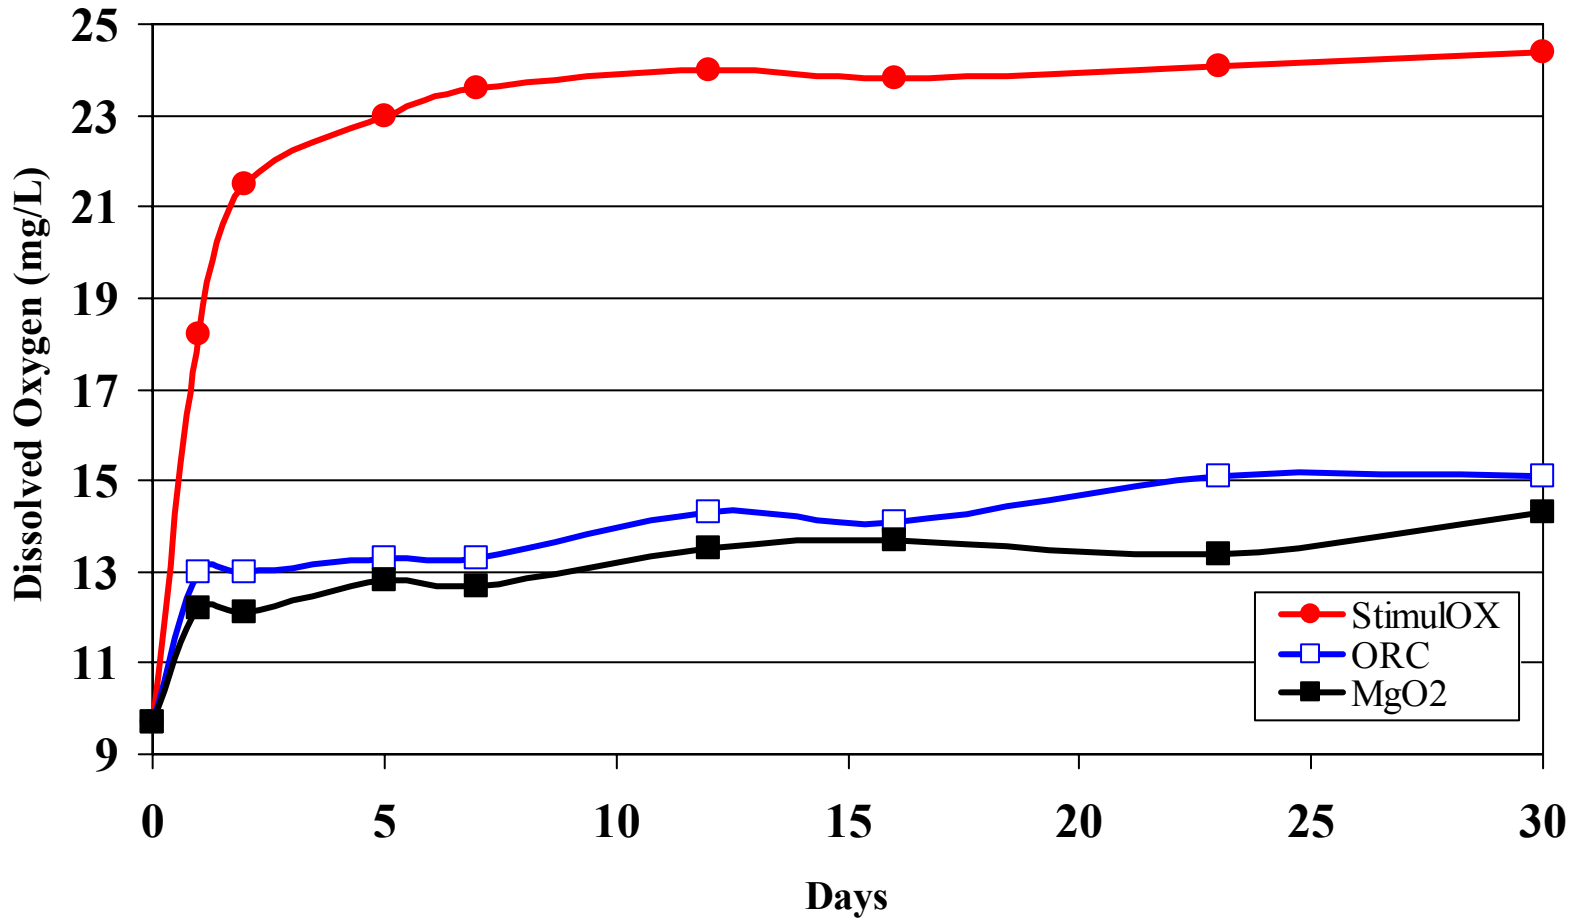


Figure 1. StimulOx Dissolved Oxygen Bench Test Results

# Comparison of StimulOX™, ORC®<sup>®</sup>, and MgO<sub>2</sub> Jar Test Solution pH

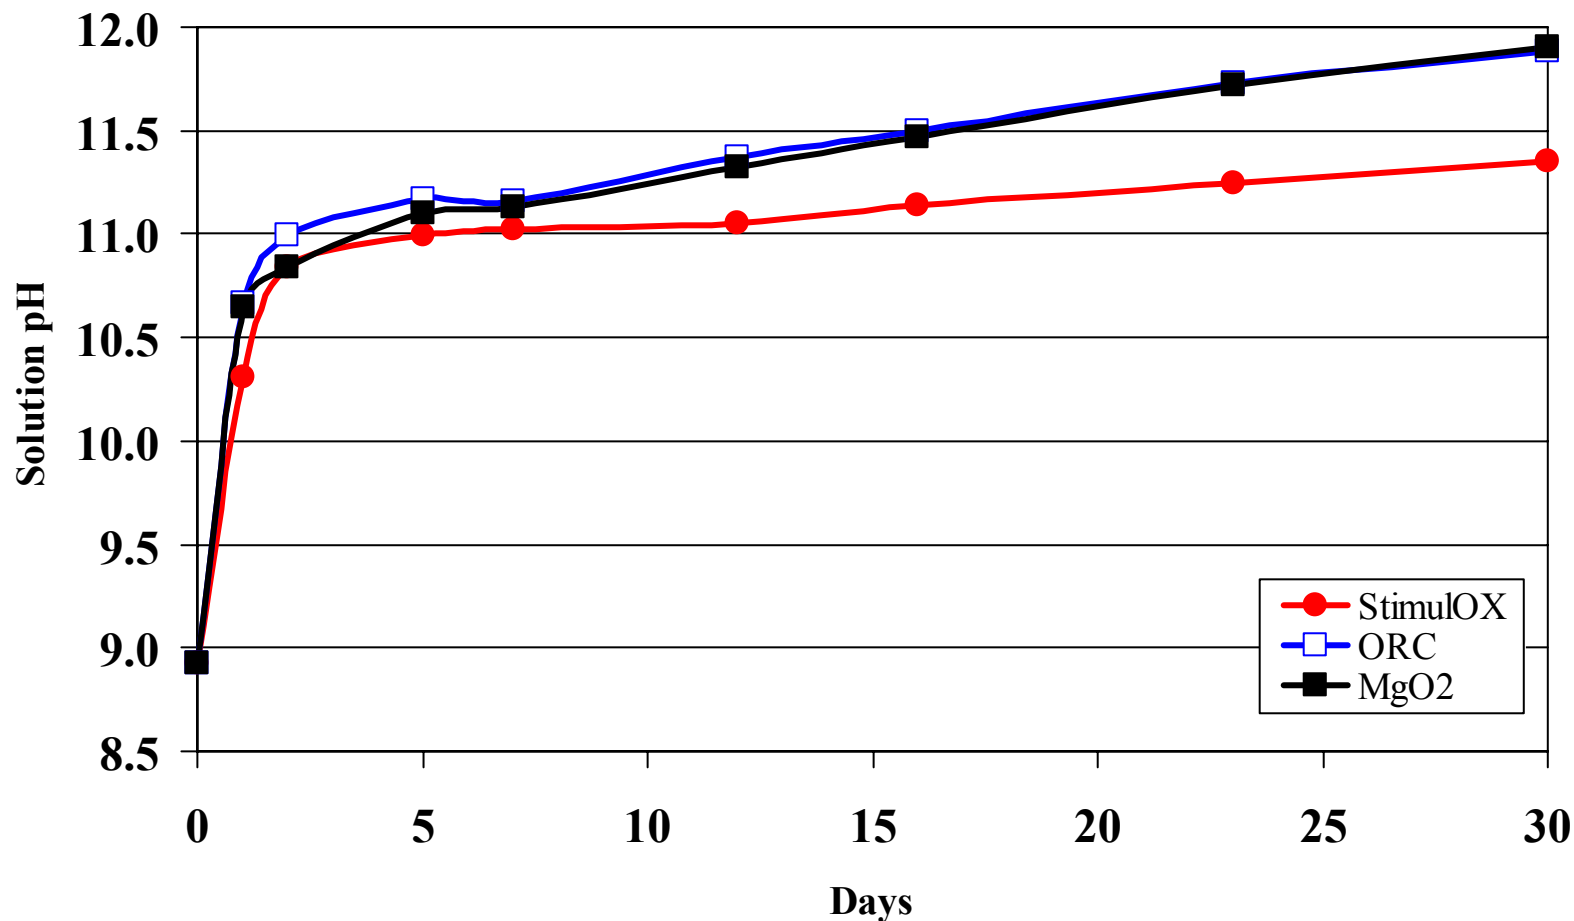
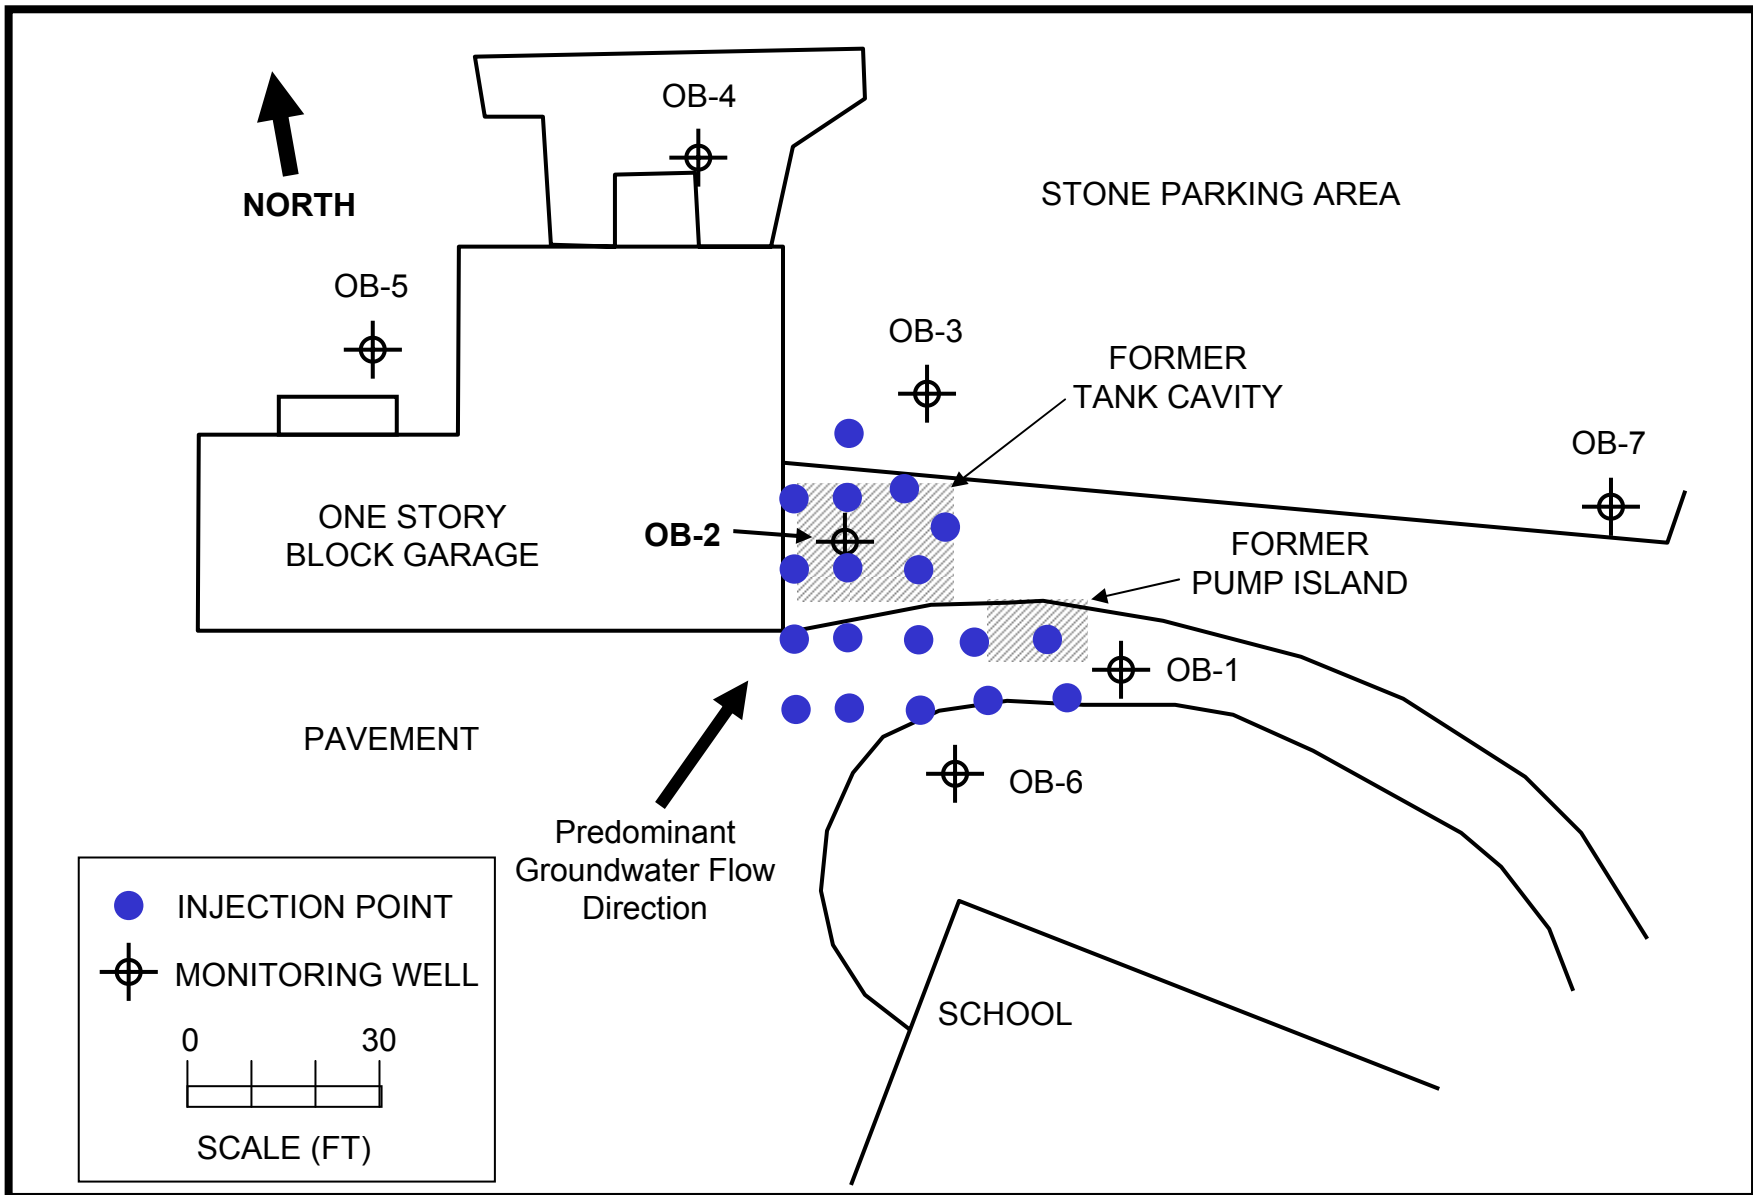


Figure 2. StimulOX™ pH Bench Test Results



**Figure 3. StimulOX™ Field Pilot Test Layout**

# Observation Well OB-2 (Source Area)

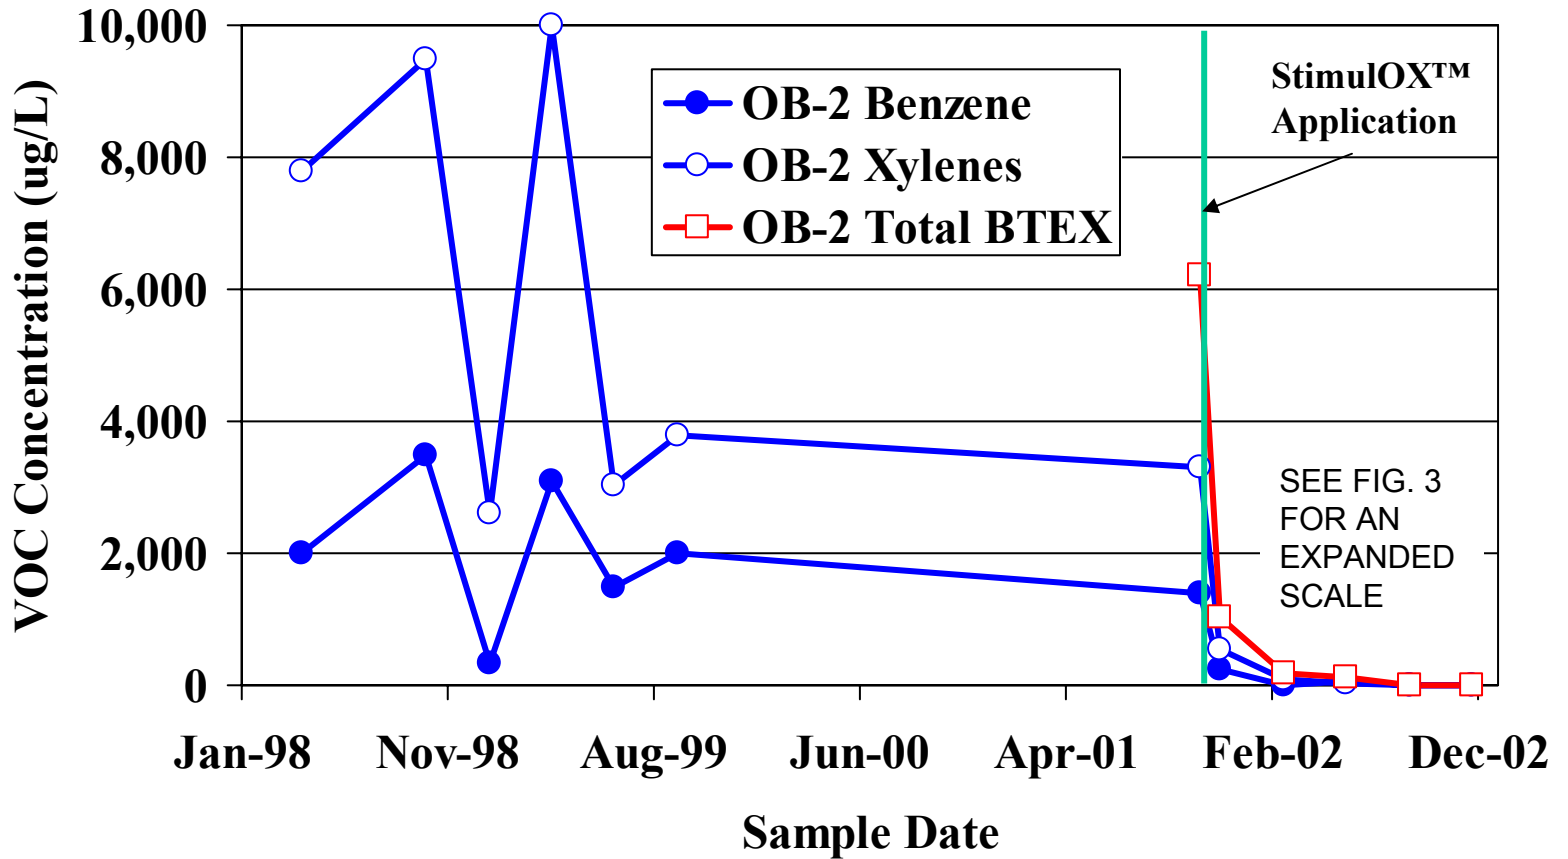


Figure 4. Historical Sampling Results for Source Area Well

# Observation Well OB-2 (Source Area)

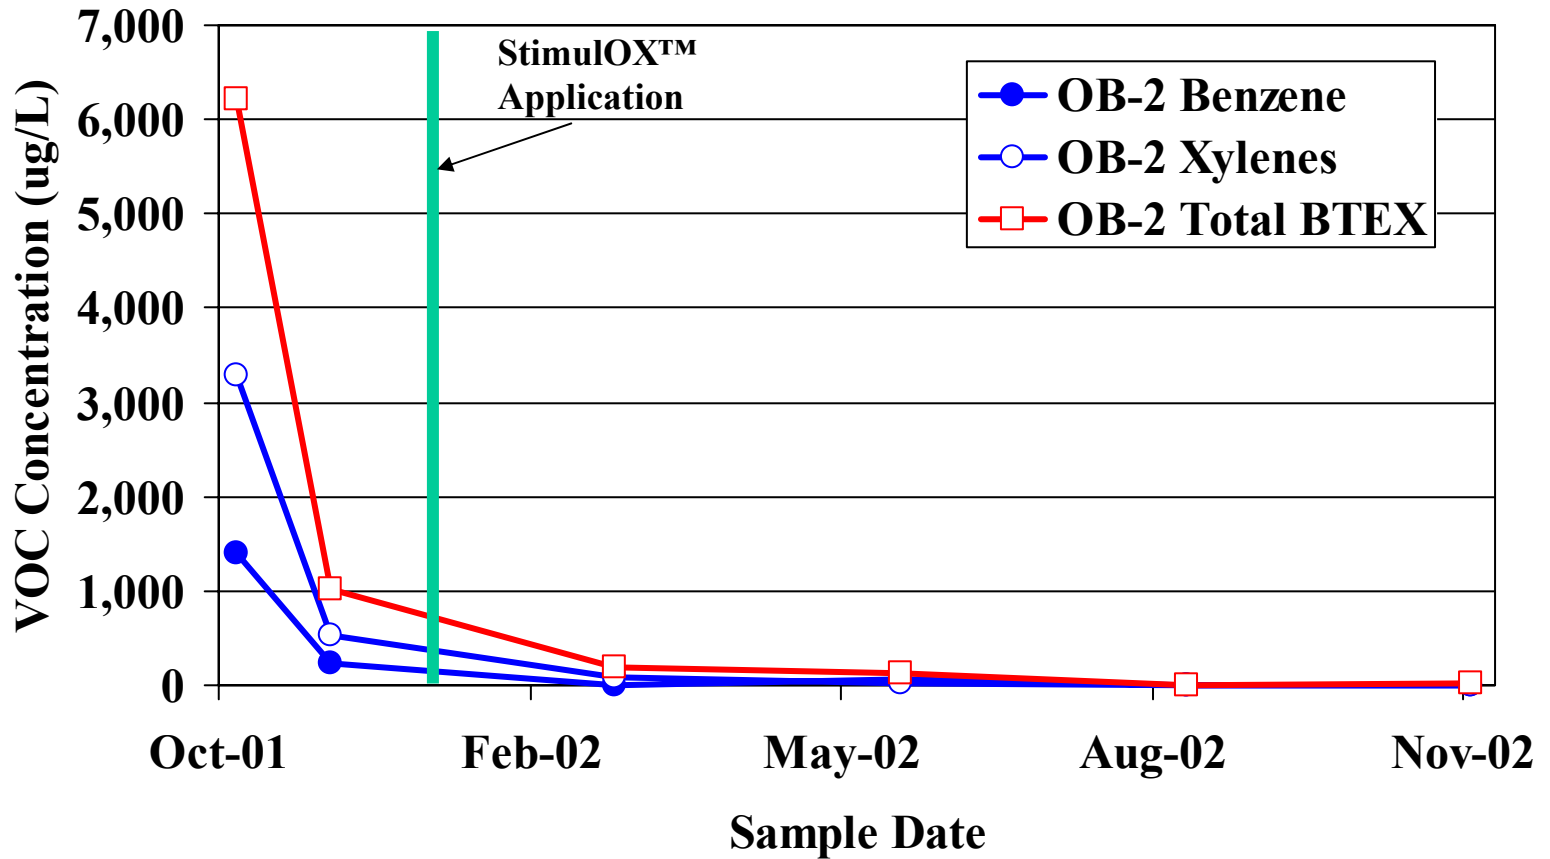


Figure 5. StimulOX™ Field Pilot Test Sampling Results for Source Area Well

# Observation Well OB-1 (Side-Gradient Well – *Outside Area of Influence*)

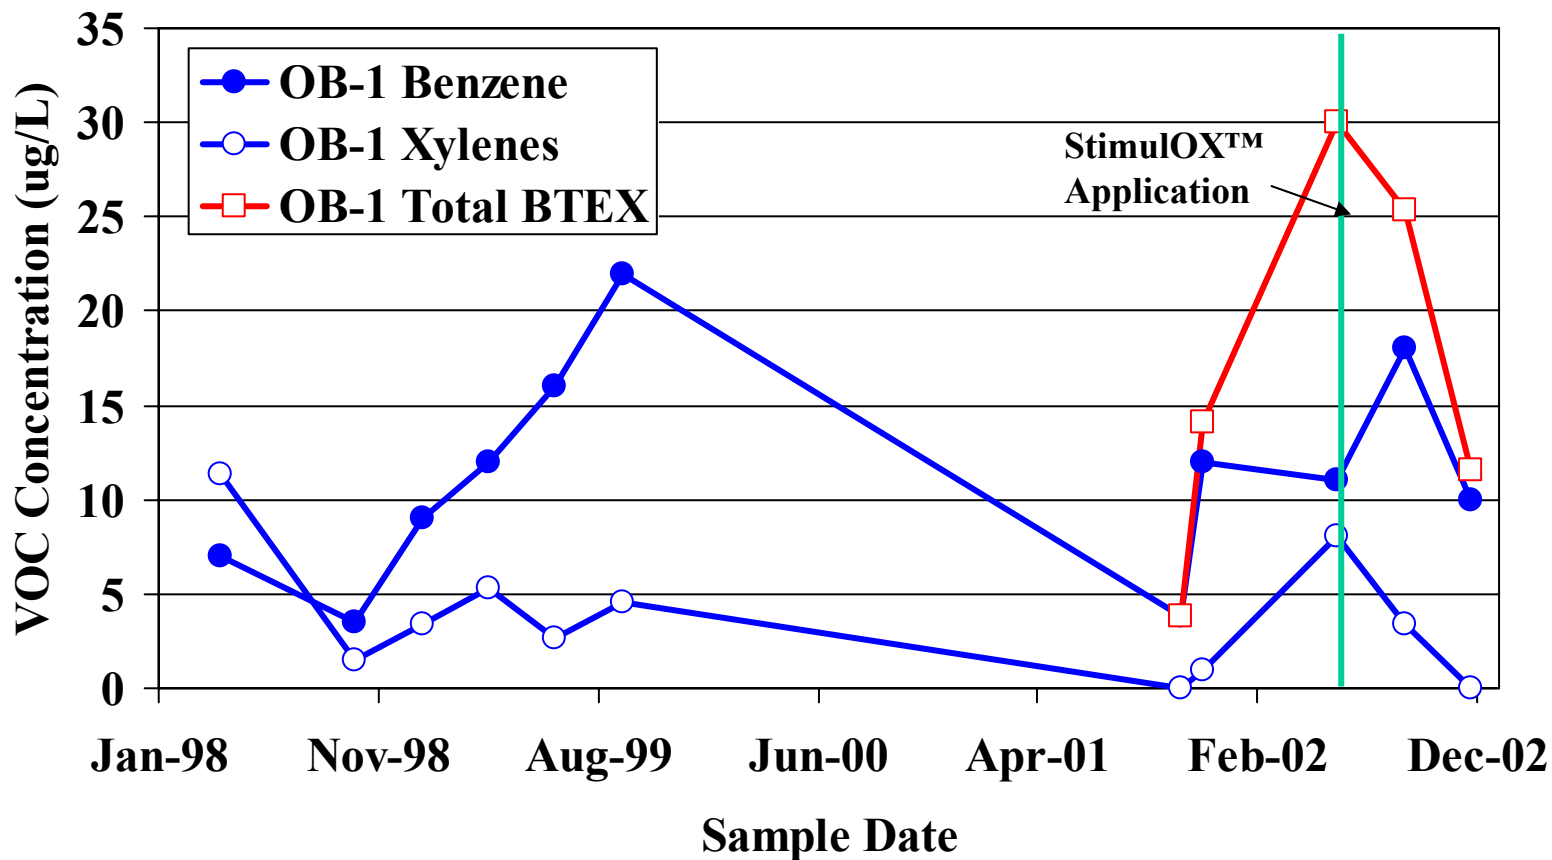


Figure 6. StimulOX™ Field Pilot Test Results for Side-Gradient Wells  
(outside of treatment area)